

## B1860-A1

### Description:


Analyzed resistance of 30 sample probes under a cycle life totaling 500,000 cycles employing a “4-wire” Kelvin test set-up.

### Tested under the following conditions:

Cycle Life- 500,000 Cycles  
Test Date-  
Tester- YOSIMURA  
Equipment- RDK Tester

### 30- Sample Probes: (mOhms)

#### **B1860-A1 TEST - 500,000 CYCLES AVERAGE RESISTANCE**

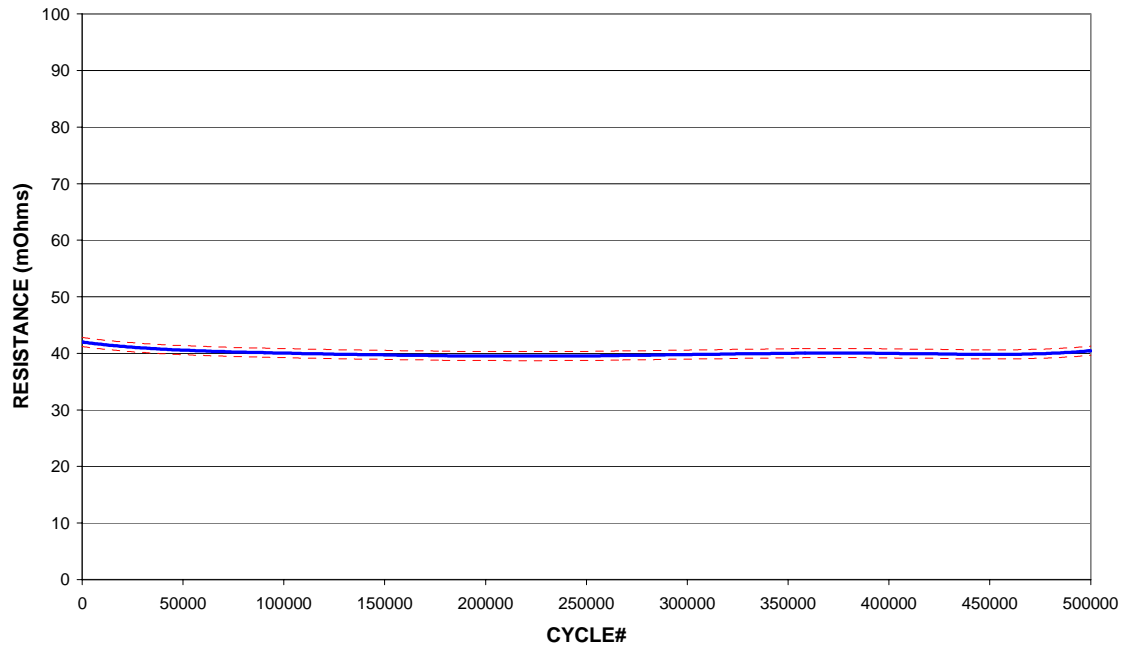

### **Summary:**

- Under a cycle program totaling 500,000 life cycles, the 30 sample probes have an average resistance of 39.99 mOhms throughout entire 500,000 life cycles. Resistance will slowly increase as cycle life increases



**RIKA DENSHI AMERICA, INC.**

112 Frank Mossberg Drive, Attleboro, MA 02703 USA

Tel: (508) 226-2080 / Toll Free: (877) 902-TEST / Fax: (508) 226-2980

Email: [mktg@testprobe.com](mailto:mktg@testprobe.com)